




Expression microarray reagent guide

Reagents



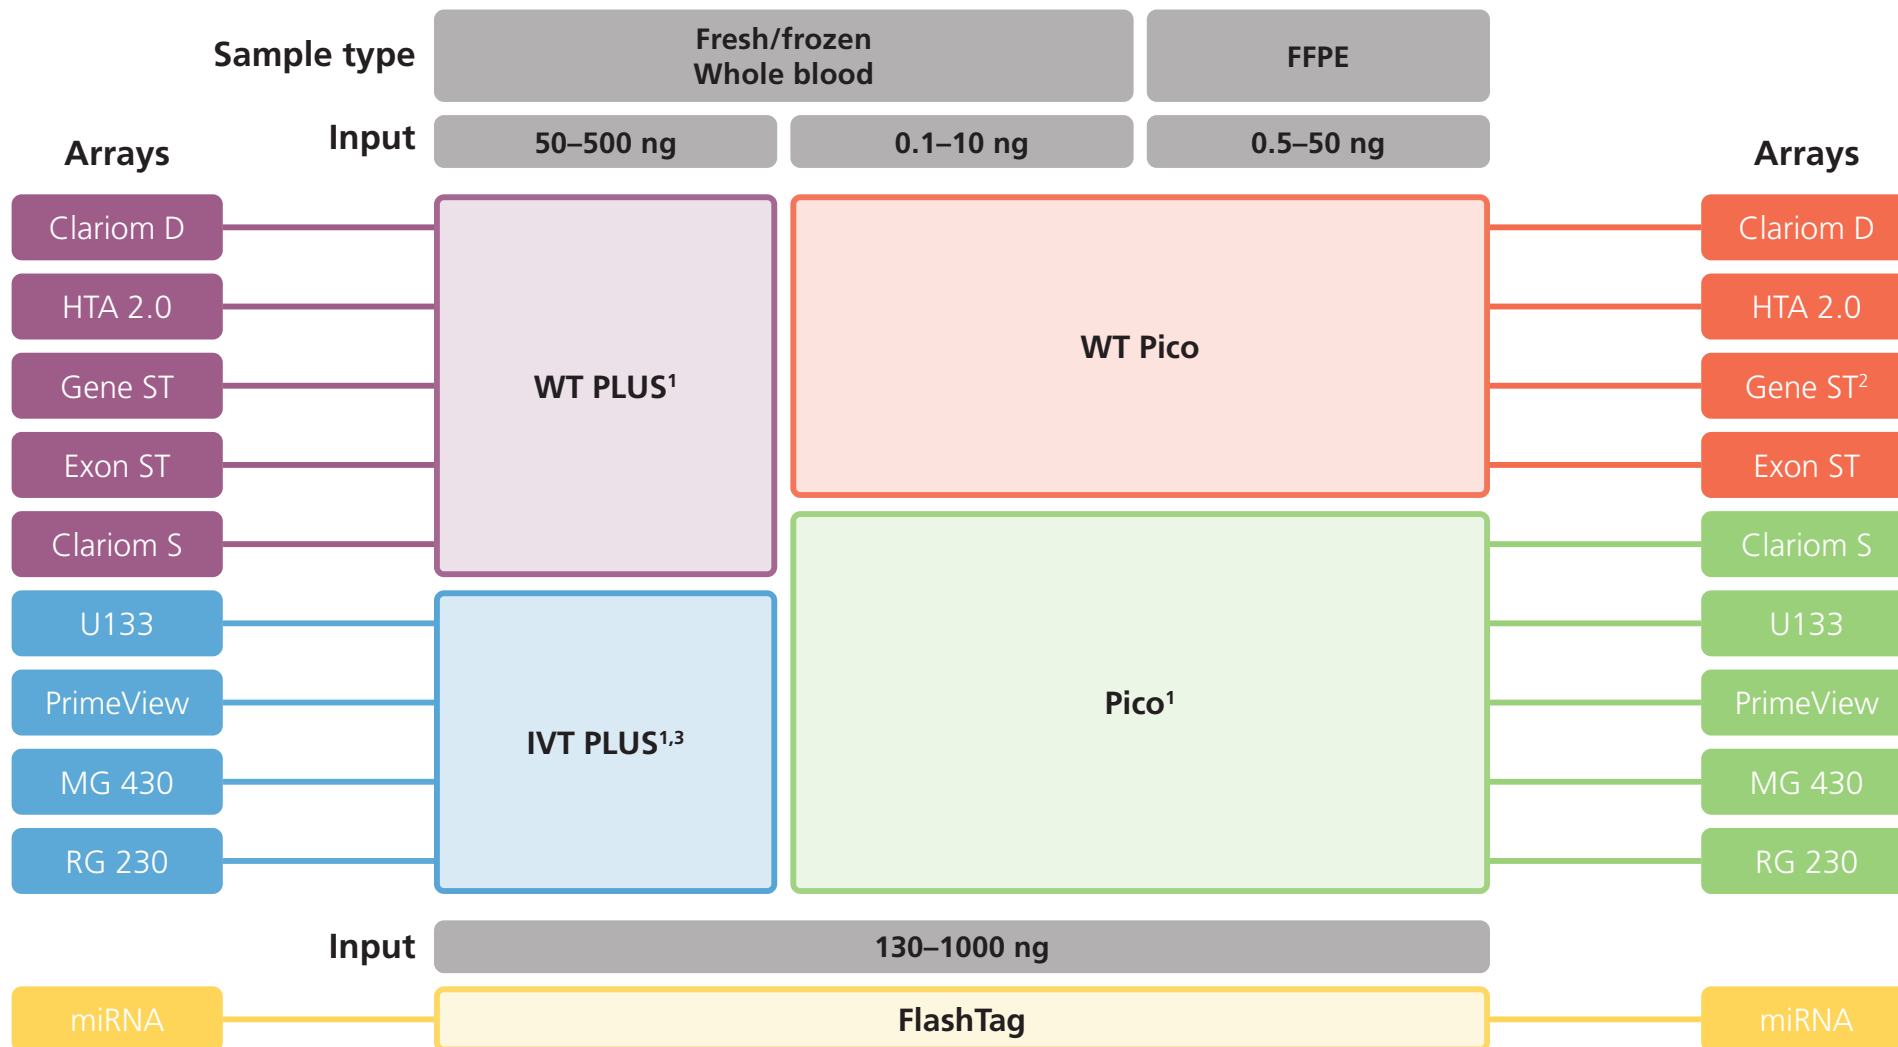

Expression microarray reagent guide

Reagents for use with microarrays

GeneChip® 3' IVT PLUS Kit (IVT PLUS) ^{1,2}	GeneChip® WT Pico Kit (WT Pico)
GeneChip® WT PLUS Reagent Kit (WT PLUS) ¹	GeneChip® Pico Kit (Pico) ¹
Affymetrix FlashTag™ Biotin HSR RNA Labeling Kit (FlashTag)	

Arrays for use with WT PLUS¹

- Clariom™ D arrays for human, mouse, and rat
- Clariom™ S arrays for human, mouse, and rat
- GeneChip® Human Transcriptome Array 2.0 (HTA 2.0)
- GeneChip® human, mouse, and rat gene ST arrays
- GeneChip® human, mouse, and rat exon 1.0 ST arrays

Arrays for use with WT Pico

- Clariom™ D arrays for human, mouse, and rat
- GeneChip® Human Transcriptome Array 2.0 (HTA 2.0)
- GeneChip® human, mouse, and rat gene ST arrays²
- GeneChip® human, mouse, and rat exon 1.0 ST arrays

Arrays for use with IVT PLUS^{1,3}

- GeneChip® Human Genome U133 Plus 2.0 Array
- GeneChip® PrimeView® Human Gene Expression Array
- GeneChip® Mouse Genome 430 2.0 Array
- GeneChip® Rat Genome 230 2.0 array

Arrays for use with Pico¹

- Clariom™ S arrays for human, mouse, and rat
- GeneChip® Human Genome U133 Plus 2.0 Array
- GeneChip® PrimeView® Human Gene Expression Array
- GeneChip® Mouse Genome 430 2.0 Array
- GeneChip® Rat Genome 230 2.0 array

Arrays for use with FlashTag

- GeneChip® miRNA arrays

List includes most common array types only and is not comprehensive. The most common arrays are paired with the appropriate reagent kits and sold as single assay part numbers for your convenience. Find additional assays, arrays, and information about the MyGeneChip™ Custom Array Program at www.affymetrix.com.

¹Also available as a high-throughput (HT) format for automation. ²Gene ST arrays should be paired with GeneChip® HT Pico Kit for automated sample preparation of challenging samples types and limited RNA input. ³Requires mRNA globin reduction for blood samples.

For Research Use Only. Not for use in diagnostic procedures.

P/N EMI06269 Rev. 2

© 2016 Affymetrix, Inc. All rights reserved. Affymetrix®, Axiom®, GeneChip®, Clariom™, CoMAP™, Command Console®, CytoScan®, DMET™, Eureka™, Eureka Genomics®, Eureka Genotyping™, Expression Console™, GeneAtlas®, GeneChip-compatible™, GeneTitan®, Genotyping Console™, myDesign™, MyGeneChip™, NetAffx®, OncoScan®, Powered by Affymetrix™, PrimeView®, and ViewRNA® are trademarks or registered trademarks of Affymetrix, Inc. Please see affymetrix.com/trademarks for a complete list of Affymetrix trademarks. All other trademarks are the property of their respective owners.